



P6 draft Spectrum Analyzer (sim).vi

Front Panel

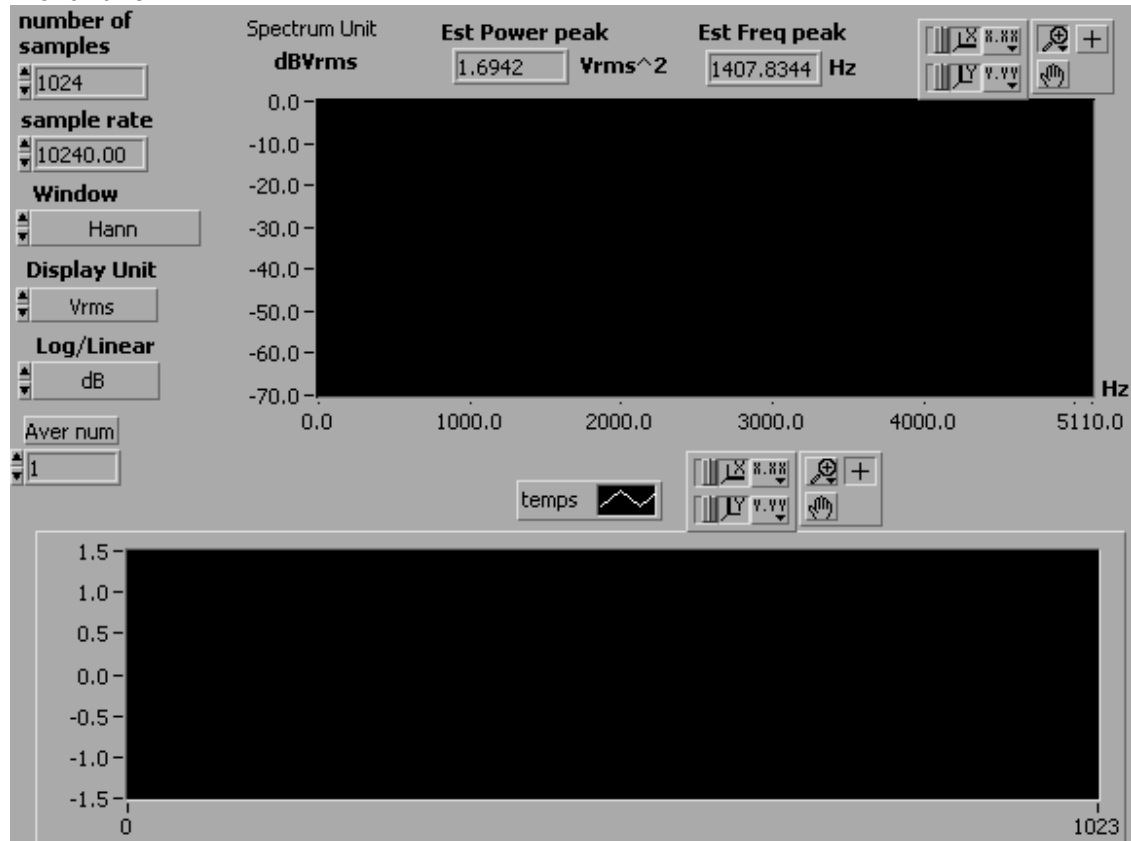


Block Diagram

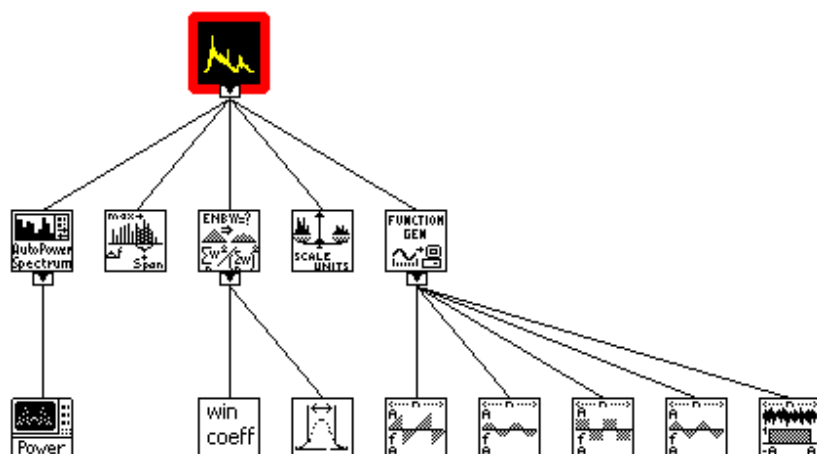


P6 adquirir del osciloscopio.vi

Front Panel

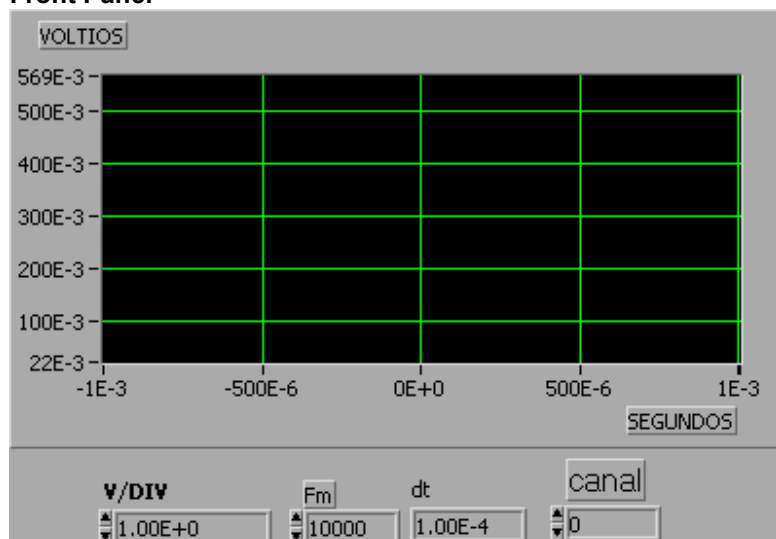

Block Diagram

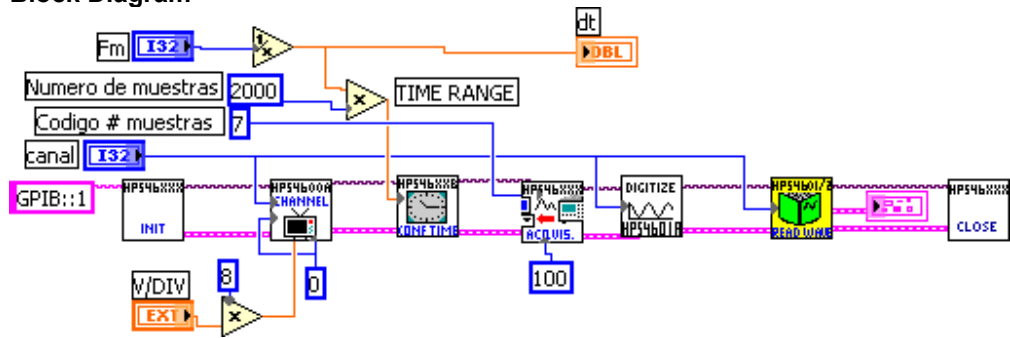

List of SubVis



HP546XXX Config Acquisition.vi

C:\Archivos de programa\National Instruments\LabVIEW
6.1\instr.lib\hp546xxx\hp546xxx.llb\HP546XXX Config Acquisition.vi



HP54601A/602B Digitize.vi

C:\Archivos de programa\National Instruments\LabVIEW
6.1\instr.lib\hp546xxx\hp546xxx.llb\HP54601A/602B Digitize.vi



HP54601A/602B Read Waveform.vi

C:\Archivos de programa\National Instruments\LabVIEW
6.1\instr.lib\hp546xxx\hp546xxx.llb\HP54601A/602B Read Waveform.vi



HP546XXX Close.vi

C:\Archivos de programa\National Instruments\LabVIEW
6.1\instr.lib\hp546xxx\hp546xxx.llb\HP546XXX Close.vi



HP54600A Channel Config.vi

C:\Archivos de programa\National Instruments\LabVIEW
6.1\instr.lib\hp546xxx\HP546XXX.LLB\HP54600A Channel Config.vi



HP546XXB Timebase Config.vi

C:\Archivos de programa\National Instruments\LabVIEW
6.1\instr.lib\hp546xxx\hp546xxx.llb\HP546XXB Timebase Config.vi



HP546XXX Initialize.vi

C:\Archivos de programa\National Instruments\LabVIEW
6.1\instr.lib\hp546xxx\hp546xxx.llb\HP546XXX Initialize.vi

Position in Hierarchy

